

Assessing Commercial Tissue-Based Assays for Autoimmune Neurologic Disorders (II)

Antibodies to Surface Antigens

Claudia Papi,^{1,2,3,*} Chiara Milano,^{1,2,4,*} Lionel Arlettaz,⁵ Pietro Businaro,^{1,6,7} Laura Marmolejo,^{1,2} Laura Naranjo,⁸ Jesús Planagumà,^{1,2} Eugenia Martínez-Hernández,^{1,2} Thaís Armangué,^{1,2,9} Mar Guasp,^{1,2} Raquel Ruiz-García,⁸ Esther Aguilar,^{1,2} Matteo Gastaldi,⁷ Raffaele Iorio,³ Carles Gaig,^{1,10} Albert Saiz,^{1,10} Lidia Sabater,^{1,2,11} Francesc Graus,¹ Josep O. Dalmau,^{1,2,10,11,12,†} and Marianna Spatola^{1,2,5,†}

Correspondence

Dr. Spatola
marianna.spatola@gmail.com

Neurol Neuroimmunol Neuroinflamm 2025;12:e200406. doi:10.1212/NXI.0000000000200406

Abstract

Background and Objectives

Detecting neural surface antibodies (NSAbs) is essential for diagnosing autoimmune encephalitis. The recommended diagnostic strategy involves initial screening with tissue-based assays (TBAs), followed by confirmation with cell-based assays (CBAs). While specialized centers use in-house TBAs, many clinical laboratories depend on commercial TBAs, whose accuracy is yet to be fully assessed.

Methods

We selected 92 CSF and 99 serum samples from patients with autoimmune encephalitis and NSAbs confirmed by in-house TBAs and CBAs (20 samples each for AMPAR, GABA_AR, GABA_BR, IgLON5, LGI1, NMDAR, and CASPR2; 19 for mGluR5; 17 for DPPX; and 15 for mGluR1 antibodies), along with 50 CSF and 50 serum samples from negative controls. We assessed the performance of a commercial indirect immunofluorescence (IIF)-TBA (EURO-IMMUN). Slides were evaluated as “positive” or “negative” by 2 experienced investigators and 2 less experienced raters. Discordant results were re-evaluated through interrater discussion and assessed using Cohen’s kappa.

Results

The experienced raters agreed on 94% (133/142) of CSF and 88% (131/149) of serum classifications (Cohen’s kappa = 0.87 and 0.75, respectively, $p < 0.001$). Among CSF samples, 75% (106/142) were correctly identified while 19% (27/142) were misclassified (13 false positives, 14 false negatives). Among serum samples, 66% (98/149) were correctly identified while 22% (33/149) were misclassified (11 false positives, 22 false negatives). The poorest performance was seen in detecting NMDAR, GABA_AR, and mGluR5 Abs, which were not identified in 5 of 10, 6 of 10, and 5 of 9 serum samples and in 4 of 10, 5 of 10, and 5 of 10 CSF samples, respectively. The overall sensitivity of the commercial IIF-TBA was 84% for CSF and 76% for serum while the specificity was 72% for CSF and 73% for serum. Less experienced raters correctly identified 69% (98/142) of CSF samples and 73% (109/149) of serum samples and misclassified 13% (18/142) of CSF samples and 11% (16/149) of serum samples, and 18% (26/142) of CSF samples and 16% (24/149) of serum samples remained discordant.

*These author contributed equally as first authors.

†These author contributed equally as senior authors.

¹Neuroimmunology Program, Fundació de Recerca Clínic Barcelona-Institut d'Investigacions Biomèdiques August Pi i Sunyer (FRCB-IDIBAPS), University of Barcelona, Spain; ²Caixa Research Institute (CRI), Barcelona, Spain; ³Department of Neuroscience, Catholic University of the Sacred Heart, Rome, Italy; ⁴Department of Clinical and Experimental Medicine, University of Pisa, Italy; ⁵Service d'Immunologie et Allergologie, Institut Central des Hôpitaux, Hôpital du Valais, Sion, Switzerland; ⁶Department of Brain and Behavioral Sciences, University of Pavia, Italy; ⁷Neuroimmunology Research Section, IRCCS Mondino Foundation, Pavia, Italy; ⁸Immunology Service, Biomedical Diagnostic Center, Hospital Clínic, Barcelona, Spain; ⁹Pediatric Neuroimmunology Unit, Neurology Department, Sant Joan de Déu Children's Hospital, ERN-RITA reference center, University of Barcelona, Spain; ¹⁰Neurology Service, Hospital Clínic de Barcelona, Spain; ¹¹Centro de Investigación Biomédica en Red, Enfermedades Raras (CIBERER), Spain; and ¹²Department of Neurology, University of Pennsylvania, PA.

The Article Processing Charge was funded by the Spanish National Institute of Health Carlos III (ISCIII) and co-funded by the European Union (Project PI23/00858).

This is an open access article distributed under the terms of the Creative Commons Attribution-Non Commercial-No Derivatives License 4.0 (CCBY-NC-ND), where it is permissible to download and share the work provided it is properly cited. The work cannot be changed in any way or used commercially without permission from the journal.

Copyright © 2025 The Author(s). Published by Wolters Kluwer Health, Inc. on behalf of the American Academy of Neurology.

e200406(1)

RELATED ARTICLES

Editorial

Beyond the Lab Slip: Why Laboratory Expertise Matters in Neuronal Antibody Testing and Why Clinicians Should Care

Page e200425

Research Article

Assessing Commercial Tissue-Based Assays for Autoimmune Neurologic Disorders (I): Antibodies to Intracellular Antigens

Page e200410

MORE ONLINE

Supplementary Material

Glossary

CBA = cell-based assay; **IHC** = immunohistochemistry; **IIF** = immunofluorescence; **NSAbs** = neural surface antibodies; **TBA** = tissue-based assay.

Discussion

The diagnostic performance of EUROIMMUN IIF-TBA in detecting NSAbs in autoimmune encephalitis is suboptimal. NMDAR antibodies, among the most common NSAbs, can be missed in 50% of cases. This commercial TBA should not be used alone as a screening method nor as a confirmatory technique for NSAbs.

Introduction

Autoimmune encephalitides are a group of disorders associated with antibodies against neural (neuronal or glial) cell-surface antigens (NSAbs).¹ The detection of NSAbs in a patient's serum and CSF is essential for diagnosing these disorders, as it confirms the suspicions raised by clinical features and paraclinical investigations.² Detection methods include immunohistochemistry (IHC) or immunofluorescence (IIF) on rodent brain tissue (tissue-based assays, TBAs), followed by confirmation of antigen specificity using cell-based assays (CBAs).^{3,4} Combination of these techniques enhances diagnostic accuracy,⁵⁻⁸ but this dual approach is rarely used in clinical laboratories, which primarily rely on CBAs or less frequently on commercially available TBAs. While some studies have evaluated the sensitivity and specificity of commercial CBAs for NSAbs detection,⁸ the accuracy of commercial TBAs remains undetermined. The aim of this study was to assess the performance of a commercially available IIF-TBA for neural surface antibody testing.

Methods

Patients, Inclusion Criteria, and Sample Selection

Patients' serum and CSF samples were obtained from the Neuroimmunology Collection (SCII number C0000051) at IDIBAPS-Hospital Clínic of Barcelona, Spain. This collection includes clinical data and samples from over 20,000 patients with suspected autoimmune neurologic disorders, referred between 2007 and 2024.

From this collection, we selected 191 samples from 148 patients with autoimmune encephalitis and NSAbs. This included 92 CSF samples (10 samples each for AMPAR, CASPR2, GABA_AR, GABA_BR, IgLON5, LGI1, mGluR5, and NMDAR; 7 for DPPX; and 5 for mGluR1 antibodies) and 99 serum samples (10 samples each for AMPAR, CASPR2, DPPX, GABA_AR, GABA_BR, IgLON5, LGI1, mGluR1, and NMDAR and 9 for mGluR5 antibodies). Patients' samples were included if they met the following criteria: (1) detection of NSAbs confirmed by 2 techniques: in-house IHC showing a characteristic pattern of reactivity with rat brain⁹ (CSF

dilution 1:2, serum dilution 1:200) and CBA confirming the specific antibody and (2) neurologic syndrome consistent with the specific antibody. Samples with multiple antibodies, including intracellular neuronal antibodies and non-neuron-specific antibodies, were excluded.

In addition, we included 50 serum and 50 CSF samples (unpaired) from 100 patients with suspected autoimmune encephalitis who tested negative for in-house TBA and CBA (negative controls). Serum and CSF samples were stored at -20°C during the study period and at -80°C for long-term storage.

Detection of Neural Surface Antibodies by Commercial IIF-TBA


A commercial IIF-TBA (EUROIMMUN—ref. FA 111a-1010-3), consisting of 2 biochips per field with fixed sections of rat hippocampus and cerebellum (both gray and white matter), was used to test all samples. Following the manufacturer's instructions, serum (dilution 1:10) and CSF (1:1) samples were incubated with the tissue at room temperature for 30 minutes. Reactivity was detected using a fluorescent anti-human antibody provided in the kit.

The results were evaluated using a Zeiss Axio Imager M2 fluorescent microscope (Carl Zeiss, Jena, Germany) by 2 expert independent raters (F.G. and J.D.) and 2 less experienced raters (C.P. and C.M.), all of whom were blinded to the in-house IHC-TBA results and clinical information. Each rater scored reactivity for neuropil staining as either "positive" or "negative." The expert raters discussed any discrepancies in their evaluations; if they reached an agreement, the result was deemed "concordant." If no agreement was reached, the result was considered "discordant." The complete study algorithm for assessment by the experienced raters is shown in Figure 1. No interrater discussion was performed between the less experienced raters.

Statistical Analysis

Categorical variables were expressed as proportions and percentages. The Cohen's kappa coefficient was used to evaluate the level of agreement on positive/negative results between the 2 expert raters and between the 2 less experienced raters. Strength of agreement was considered according

Figure 1 Algorithm of the Study

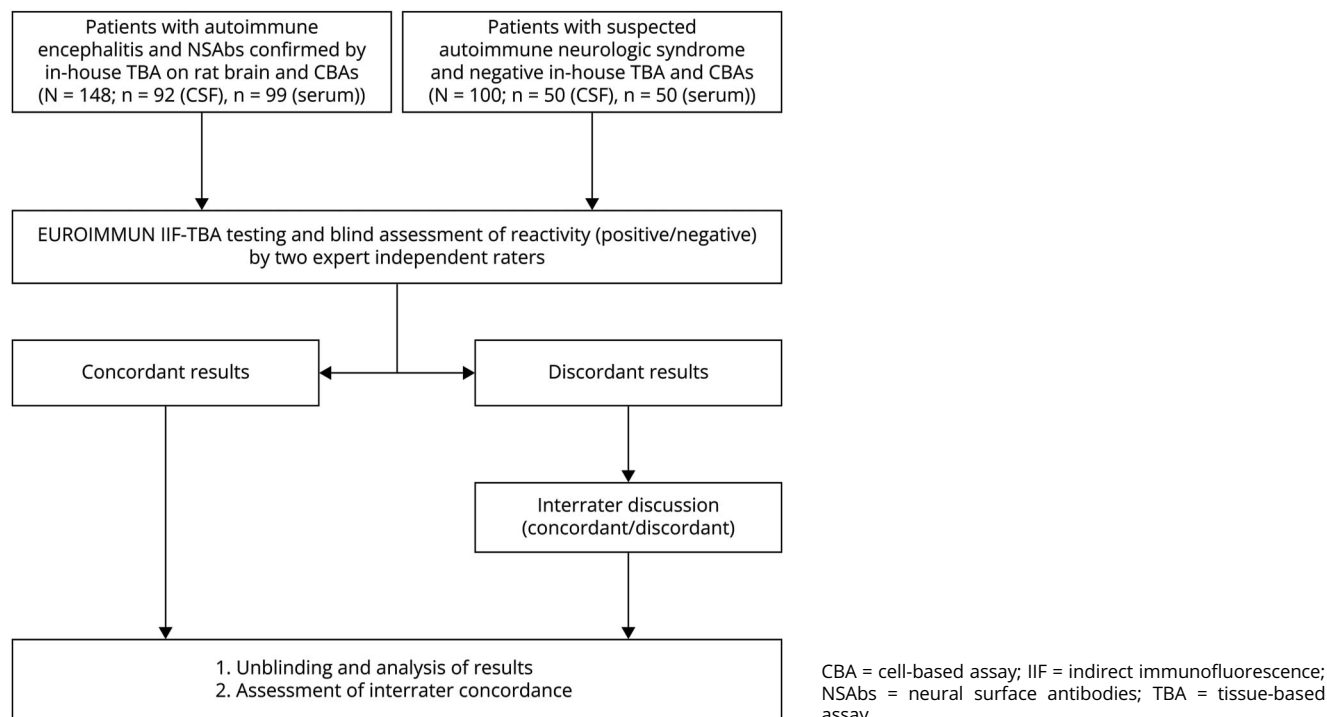

to the kappa index value, as reported¹⁰ (<0.40 was considered poor concordance, 0.41–0.57 fair, 0.58–0.75 good, and >0.75 excellent). The percentages of true/false-positive/negative results were calculated separately for serum and CSF samples. Sensitivity and specificity were determined after excluding samples with discordant results and were expressed as percentages with 95% confidence intervals. Statistical analyses were conducted using IBM SPSS Statistics 20.

Standard Protocol Approvals, Registrations, and Patient Consents

The study was approved by the Institutional Review Board of the Hospital Clínic, Barcelona (Reg. HCB/2023/1183). All patients or their proxies provided written informed consent for the storage and use of serum, CSF, and clinical information for research purposes.

Data Availability

Anonymized participant data can be shared with qualified investigators on request to the corresponding author.

Results

Clinical Syndromes, Rater Concordance, and Performance of the Commercial IIF-TBA in CSF Samples

The demographics, clinical syndromes, and associated tumors of the 148 patients with NSAbs were consistent with the expected features for each antibody, as summarized in eTable 1.

Regarding CSF samples, the 2 experienced raters agreed on the negative/positive results in 69% (98/142) of cases (Cohen's kappa = 0.40, $p < 0.001$). After re-evaluating the discordant samples, they reached a consensus for 94% (133/142) of the samples, showing excellent agreement (Cohen's kappa = 0.87, $p < 0.001$), with 9 samples remaining discordant. Overall, using the commercial IIF-TBA, 75% (106/142) of the CSF samples were correctly identified (true positive/negative), 19% (27/142) were misclassified (false positive/negative), and 6% (9/142) remained discordant (Figure 2).


When considering only the antibody-positive samples, 78% (72/92) were correctly identified as positives, 15% (14/92) were misclassified as false negatives, and 7% (6/92) remained discordant (Figure 2).

Among the negative control CSF samples, 68% (34/50) were correctly identified as negatives, 26% (13/50) were misclassified as false positives, and 6% (3/50) remained discordant (Figure 2).

The overall sensitivity of the commercial IIF-TBA for CSF samples was 84% (95% CI 74.2%–90.8%), and its specificity was 72% (95% CI 57.4%–84.4%).

Less experienced raters agreed in 82% (116/142) of the cases (Cohen's kappa = 0.53, $p < 0.001$; no interrater discussion was performed), correctly identifying 69% (98/142) and misclassifying 13% (18/142). 18% (26/142) of the samples remained discordant (not shown).

Figure 2 Pie Charts Showing the Percentages of True/False-Positive/Negative Results in CSF (A) and Serum (B) Samples Using EUROIMMUN IIF-TBA

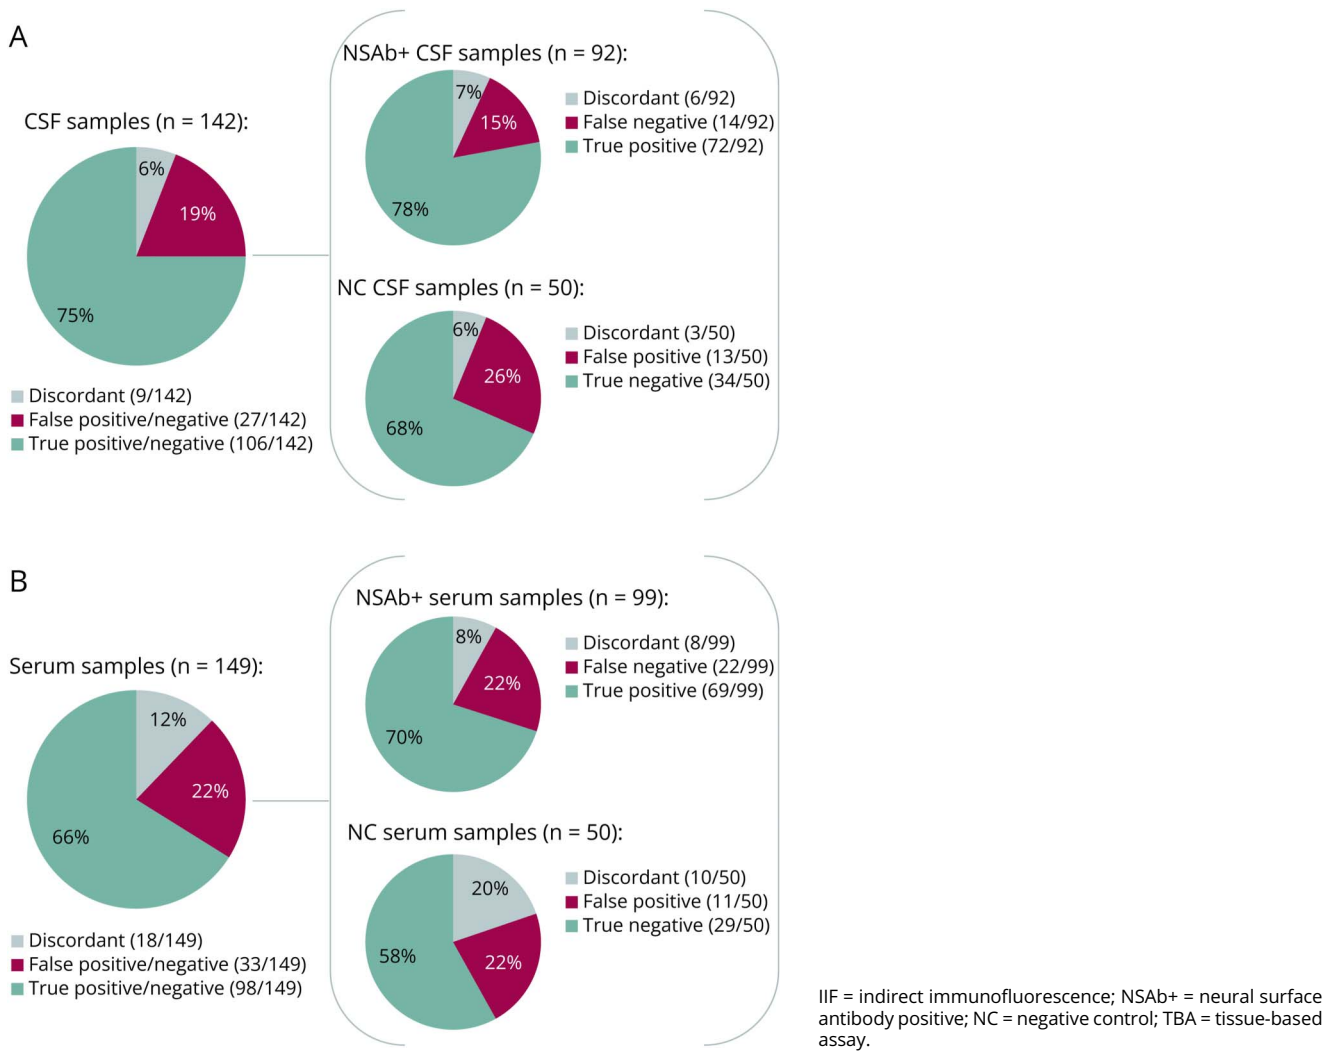

Rater Concordance and Performance Evaluation of the Commercial IIF-TBA in Serum Samples

For serum samples, the 2 experienced raters initially agreed in 64% (96/149) of cases (Cohen's kappa = 0.32, $p < 0.001$). After re-evaluating the discordant samples, they reached a consensus for 88% (131/149) of the samples, showing good agreement (Cohen's kappa = 0.75, $p < 0.001$), with 18 samples remaining discordant.

Overall, using the commercial IIF-TBA, 66% (98/149) of the serum samples were correctly identified as true positives/negatives, 22% (33/149) were misclassified as false positives/negatives, and 12% (18/149) remained discordant (Figure 2). When considering only the antibody-positive samples, 70% (69/99) were classified as true positives, 22% (22/99) were misclassified as false negatives, and 8% (8/99) remained discordant (Figure 2).

Among the negative control serum samples, 58% (29/50) were correctly identified as negatives, 22% (11/50) were misclassified as false positives, and 20% (10/50) remained discordant (Figure 2).

The overall sensitivity of the commercial IIF-TBA for serum samples was 76% (95% CI 65.7%–84.2%), and its specificity was 73% (95% CI 56.1%–85.4%).

Less experienced raters agreed in 84% (125/149) of the cases (Cohen's kappa = 0.63, $p < 0.001$; no interrater discussion was performed), correctly identifying 73% (109/149) and misclassifying 11% (16/149). 16% (24/149) of the samples remained discordant (not shown).

Performance of the Commercial IIF-TBA in Detecting Specific Neural Antibodies

The antibody-specific pattern of hippocampal and cerebellar staining typically observed with in-house TBAs was not

always detectable using the commercial IIF-TBA (Figure 3). Therefore, this section focuses on the positive/negative results for each antibody-positive sample (Figure 4), without considering the specific pattern of reactivity.

The detection of certain antibodies by the 2 experienced raters was optimal for both CSF and serum samples. For instance, DPPX antibodies were identified as positive in all samples: 7 of 7 CSF and 10 of 10 serum samples. Similarly, high performance was observed for CASPR2, GABA_BR, and mGluR1 antibodies, which were correctly identified in 9 of 10, 9 of 10, and 4 of 5 CSF samples and in 9 of 10, 8 of 10, and 8 of 10 serum samples, respectively.

However, the performance varied for other antibodies between serum and CSF. For example, IgLON5 and LGI1


antibodies were identified in all CSF samples (10/10), but only in 7 of 10 (IgLON5) and 4 of 10 (LGI1) serum samples. Conversely, AMPAR antibodies were better identified in serum (10/10) than in CSF (7/10).

The lowest performance was observed for NMDAR, GABA_AR, and mGluR5 antibodies, which were correctly identified in 6 of 10, 5 of 10, and 5 of 10 CSF samples and in 5 of 10, 4 of 10, and 4 of 9 serum samples, respectively.

Discussion

This study evaluated the diagnostic yield of a commercial IIF-TBA in detecting NSAbs. We included 191 samples from

Figure 3 Examples of NMDAR and LGI1 Antibody Staining on In-House IHC and Commercial IIF-TBA

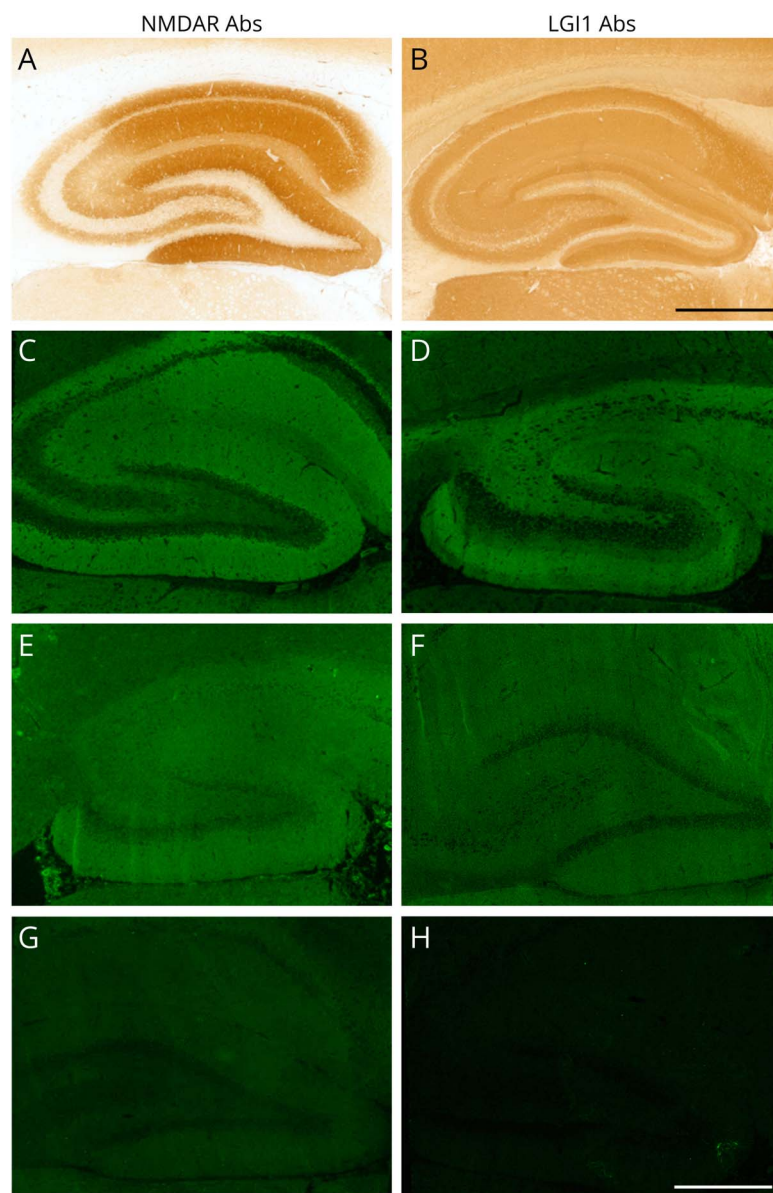

Staining patterns of samples positive for NMDAR (left column) and LGI1 (right column) antibodies on rat hippocampus with in-house IHC and IIF-TBA. Characteristic staining patterns of NMDAR (A) and LGI1 (B) antibodies with in-house IHC. In some cases, the same recognizable typical staining pattern was observed on IIF-TBA (C, D), whereas in others, the sample was labeled as “positive” although a typical staining pattern was not observed (E, F). Examples of NMDAR (G) and LGI1 (H) antibody-positive samples with negative staining with IIF-TBA. Scale bar = 500 μ m. Abs = antibodies; IHC = immunohistochemistry; IIF = indirect immunofluorescence; LGI1 = leucine-rich glioma inactivated 1; NMDAR = N-methyl-D-aspartate receptor; TBA = tissue-based assay.

(1) Low neural autoantibody titers may not be detected by the commercial IIF-TBA, as suggested in a previous study.¹⁵ However, we did not observe significant differences in staining intensity on in-house IHC between true-positive and false-negative samples by the commercial IIF-TBA (data not shown). (2) The inclusion of selected brain regions (cerebellum and hippocampus only) in the commercial IIF-TBA mosaics, compared with the whole rodent brain in in-house IHC, may limit the diagnostic evaluation. (3) Antibody epitope specificity may be affected by the tissue processing and fixation of certain antigens, contributing to false-negative results.

In conclusion, our study suggests that the commercial IIF-TBA has limitations in detecting antibodies against neural surface antigens and should not be recommended as a screening test (or as confirmatory test) for autoimmune encephalitis. In this clinical setting, specific confirmatory tests (CBA for NSAbs) become the primary diagnostic tools. However, given that previous studies have identified challenges with some of these tests,^{8,16} we recommend referring patient samples to specialized neuroimmunology laboratories where in-house diagnostic techniques (TBAs and CBAs) are available. This is particularly important in cases of high clinical suspicion despite a negative result on the commercial IIF-TBA, especially if the commercial CBA is negative or results are incongruent with the clinical syndrome.

Acknowledgment

The authors thank EUROIMMUN for providing the TBA kits.

Author Contributions

C. Papi: drafting/revision of the manuscript for content, including medical writing for content; major role in the acquisition of data; analysis or interpretation of data. C. Milano: drafting/revision of the manuscript for content, including medical writing for content; major role in the acquisition of data; analysis or interpretation of data. L. Arlettaz: drafting/revision of the manuscript for content, including medical writing for content. P. Businaro: drafting/revision of the manuscript for content, including medical writing for content. L. Marmolejo: drafting/revision of the manuscript for content, including medical writing for content. L. Naranjo: drafting/revision of the manuscript for content, including medical writing for content. J. Planagumà: drafting/revision of the manuscript for content, including medical writing for content. E. Martínez-Hernández: drafting/revision of the manuscript for content, including medical writing for content. T. Armangue: drafting/revision of the manuscript for content, including medical writing for content. M. Guasp: drafting/revision of the manuscript for content, including medical writing for content. R.R. García: drafting/revision of the manuscript for content, including medical writing for content. E. Aguilar: drafting/revision of the manuscript for content, including medical writing for content. M. Gastaldi: drafting/revision of the manuscript for content, including medical writing for content. R. Iorio: drafting/revision of the

manuscript for content, including medical writing for content. C. Gaig: drafting/revision of the manuscript for content, including medical writing for content. A. Saiz: drafting/revision of the manuscript for content, including medical writing for content. L. Sabater: drafting/revision of the manuscript for content, including medical writing for content. F. Graus: drafting/revision of the manuscript for content, including medical writing for content; major role in the acquisition of data; study concept or design; analysis or interpretation of data. J.O. Dalmau: drafting/revision of the manuscript for content, including medical writing for content; major role in the acquisition of data; study concept or design; analysis or interpretation of data. M. Spatola: drafting/revision of the manuscript for content, including medical writing for content; major role in the acquisition of data; study concept or design; analysis or interpretation of data.

Study Funding

The authors report no targeted funding.

Disclosure

C. Papi receives research support from Spanish National Health Institute Carlos III (FIS grant PI23/01366) and 2023 EAN Research Training Fellowship. C. Milano receives research support from Spanish National Health Institute Carlos III co-funded by the European Union (Rio-Hortega grant CM24/00055). L. Marmolejo receives research support from Spanish National Health Institute Carlos III (predoctoral research grant FI24/00021). M. Spatola receives research support from La Caixa Foundation (Junior Leader) and Spanish National Health Institute Carlos III (ISCIII) and co-funded by the European Union (FIS grant PI23/01366). J. Dalmau receives research support from CaixaResearch Health 2022 (HR22-00221), Spanish National Health Institute Carlos III (ISCIII) and co-funded by the European Union (FIS grant PI23/00858), Cellex Foundation, Fundació Clínic per a la Recerca Biomèdica (FCRB) Programa Multidisciplinar de Recerca, Generalitat de Catalunya Department of Health (SLT028/23/000071), Edmond J. Safra Foundation. He receives royalties from Euroimmun for the use of NMDA as an antibody test. He received a licensing fee from Euroimmun for the use of GABAB receptor, GABAA receptor, DPPX and IgLON5 as autoantibody tests. He has received a research grant from Sage Therapeutics. All the other authors report no disclosures relevant to the manuscript. Go to [Neurology.org/NN](https://www.neurology.org/NN) for full disclosures.

Publication History

Received by *Neurology*[®] *Neuroimmunology & Neuroinflammation* January 31, 2025. Accepted in final form March 19, 2025. Submitted and externally peer reviewed. The handling editor was Romana Höftberger, MD.

References

1. Dalmau J, Graus F. Antibody-mediated encephalitis. *N Engl J Med*. 2018;378(9):840-851. doi:10.1056/NEJMra1708712
2. Graus F, Titulaer MJ, Balu R, et al. A clinical approach to diagnosis of autoimmune encephalitis. *Lancet Neurol*. 2016;15(4):391-404. doi:10.1016/S1474-4422(15)00401-9
3. Höftberger R, Dalmau J, Graus F. Clinical neuropathology practice guide 5-2012: updated guideline for the diagnosis of antineuronal antibodies. *Clin Neuropathol*. 2012;31(5):337-341. doi:10.5414/np300545

4. Dalmau J, Graus F. Diagnostic criteria for autoimmune encephalitis: utility and pitfalls for antibody-negative disease. *Lancet Neurol.* 2023;22(6):529-540. doi:10.1016/S1474-4422(23)00083-2
5. Gresa-Arribas N, Titulaer MJ, Torrents A, et al. Antibody titres at diagnosis and during follow-up of anti-NMDA receptor encephalitis: a retrospective study. *Lancet Neurol.* 2014;13(2):167-177. doi:10.1016/s1474-4422(13)70282-5
6. Spatola M, Petit-Pedrol M, Simabukuro MM, et al. Investigations in GABAA receptor antibody-associated encephalitis. *Neurology.* 2017;88(11):1012-1020. doi:10.1212/WNL.0000000000003713
7. Kerstens J, Schreurs MWJ, de Vries JM, et al. Autoimmune encephalitis and paraneoplastic neurologic syndromes: a nationwide study on epidemiology and antibody testing performance. *Neurol Neuroimmunol Neuroinflamm.* 2024;11(6):e200318. doi:10.1212/nxi.00000000000200318
8. Ruiz-García R, Muñoz-Sánchez G, Naranjo L, et al. Limitations of a commercial assay as diagnostic test of autoimmune encephalitis. *Front Immunol.* 2021;12:691536. doi:10.3389/fimmu.2021.691536
9. Dalmau J, Geis C, Graus F. Autoantibodies to synaptic receptors and neuronal cell surface proteins in autoimmune diseases of the central nervous system. *Physiol Rev.* 2017;97(2):839-887. doi:10.1152/physrev.00010.2016
10. Cicchetti DV, Sparrow SA. Developing criteria for establishing interrater reliability of specific items: applications to assessment of adaptive behavior. *Am J Ment Defic.* 1981;86(2):127-137.
11. Titulaer MJ, McCracken L, Gabilondo I, et al. Treatment and prognostic factors for long-term outcome in patients with anti-NMDA receptor encephalitis: an observational cohort study. *Lancet Neurol.* 2013;12(2):157-165. doi:10.1016/s1474-4422(12)70310-1
12. Graus F, Vogrig A, Muñoz-Castrillo S, et al. Updated diagnostic criteria for paraneoplastic neurologic syndromes. *Neurol Neuroimmunol Neuroinflamm.* 2021;8(4):e1014. doi:10.1212/NXI.0000000000001014
13. Armangue T, Spatola M, Vlaga A, et al. Frequency, symptoms, risk factors, and outcomes of autoimmune encephalitis after herpes simplex encephalitis: a prospective observational study and retrospective analysis. *Lancet Neurol.* 2018;17(9):760-772. doi:10.1016/S1474-4422(18)30244-8
14. Zuliani L, Marangoni S, De Gaspari P, et al. Epidemiology of neuronal surface antibody-mediated autoimmune encephalitis and antibody-based diagnostics. *J Neuroimmunol.* 2021;357:577598. doi:10.1016/j.jneuroim.2021.577598
15. Nagata N, Kanazawa N, Mitsuhata T, et al. Neuronal surface antigen-specific immunostaining pattern on a rat brain immunohistochemistry in autoimmune encephalitis. *Front Immunol.* 2022;13:1066830. doi:10.3389/fimmu.2022.1066830
16. Muñoz-Sánchez G, Planagumà J, Naranjo L, et al. The diagnosis of anti-LGI1 encephalitis varies with the type of immunodetection assay and sample examined. *Front Immunol.* 2022;13:1069368. doi:10.3389/fimmu.2022.1069368